

Scaled data based on original data using
LM-79-08 Approved Method: Electrical and Photometric Measurements of Solid-State
Lighting Products

Test Report Prepared for

Cooper Lighting Solutions

(formerly Eaton)

Brand: FAIL-SAFE

Report Number: P696920

Luminaire Tested: **MRI-FEU4C-25-L935 F4X-N-X-LI**

Issue Date: 08/03/2023



Test Information

Test Method: LM-79-08
Report Number: P696920
TEST IS SCALED FROM IESNA LM-79-08 TEST DATA (P208279)
Test Lab: INNOVATION CENTER-P3
Issue Date: 08/03/2023
Manufacturer: COOPER LIGHTING SOLUTIONS (FORMERLY EATON)
Product Line: FAIL-SAFE
Catalog Number: MRI-FEU4C-25-L935 F4X-N-X-LI
Description: 4 INCH FAIL-SAFE MRI LED DOWNLIGHT WITH 3500K, 90 CRI LEDS, 4LBNLI TRIM
Light Source: -
Ballast/Driver: -


Summary

Lumens per Lamp: N/A
Luminaire Lumens: 2193.0 lumens
Efficiency: N/A
Efficacy: 69.4 lumens/watt
Spacing Criteria (0/90/45): 0.48 / 0.48 / 0.54
Luminous Opening: Circular (Dia: 0.33' x H: 0')
CIE Type: Direct

Input Watts (W): 31.6
Input Voltage (V): NR
Input Current (Ain): NR
Voltage Rise (V): NR
Power Factor: NR
Total Harmonic Distortion (THDi): NR
Frequency (hertz): 60
Stabilization Time: NR
Operation Time: NR
Ambient Temperature (°C): NR
Test Distance: 25 FT

TEST NUMBER: P696920
CATALOG NUMBER: MRI-FEU4C-25-L935 F4X-N-X-LI

Luminous Intensity Polar Plot

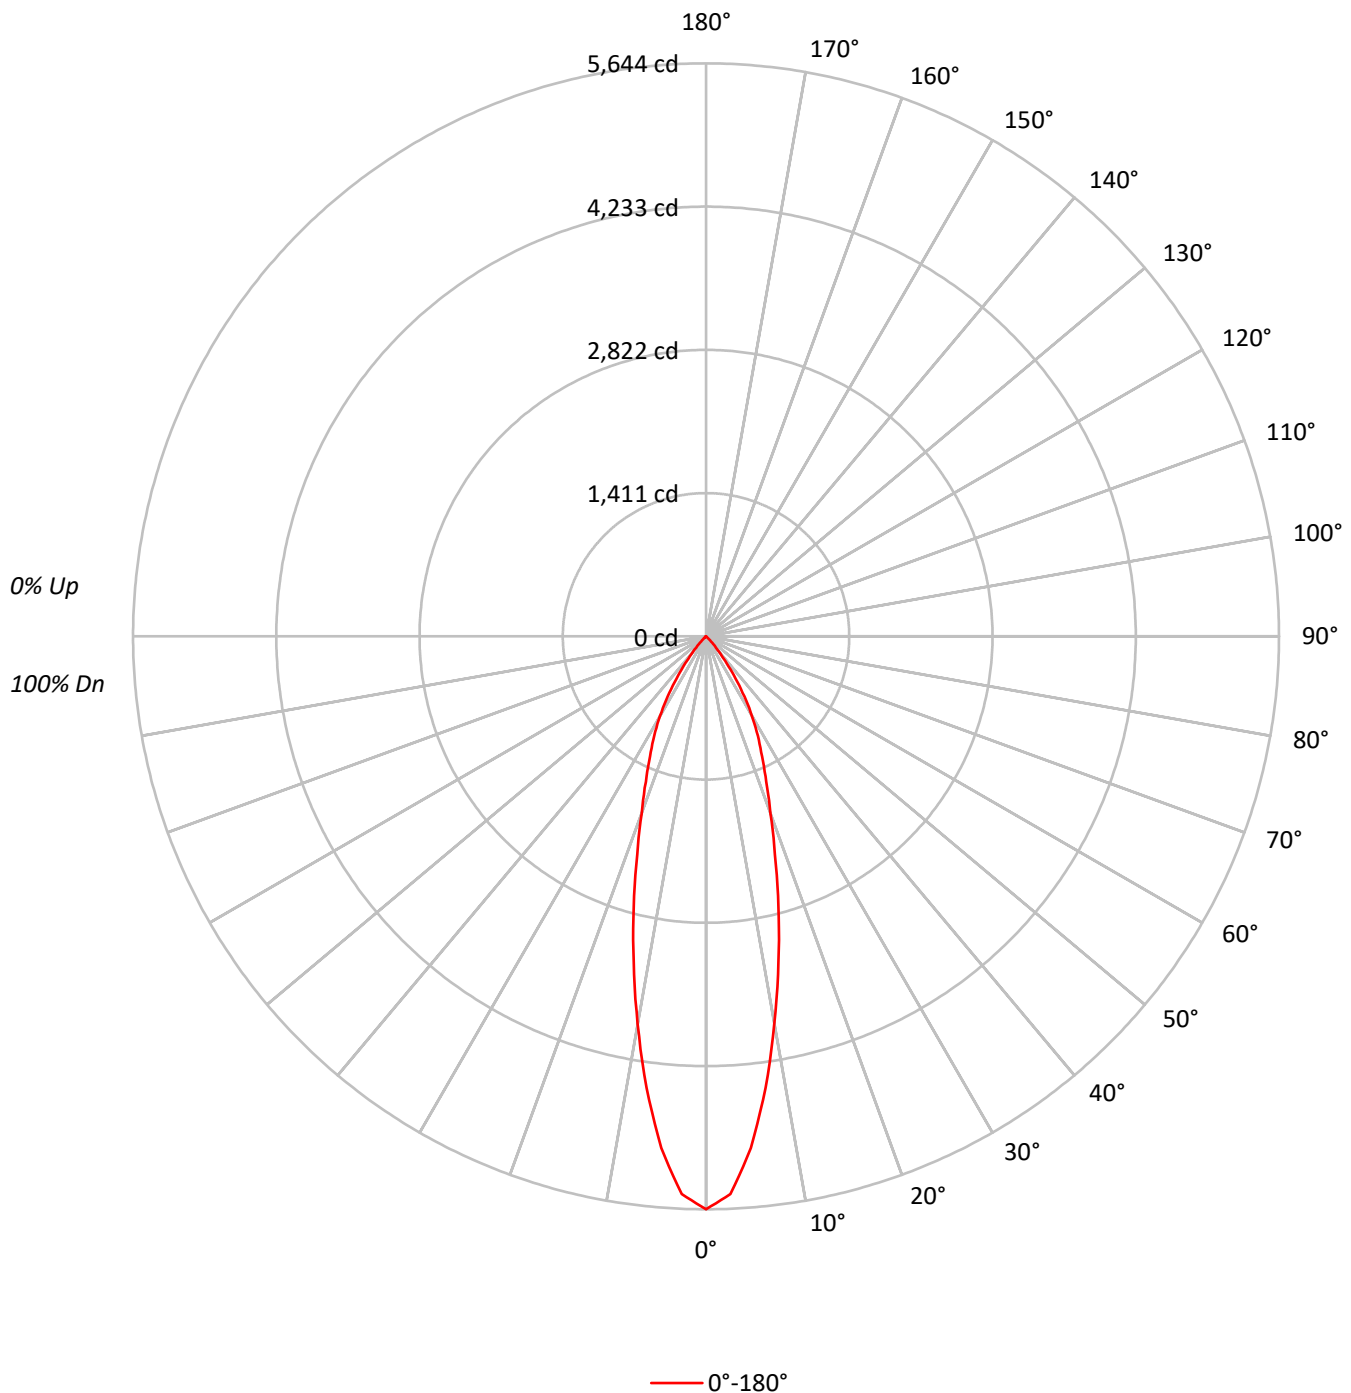



TEST NUMBER: P696920

CATALOG NUMBER: MRI-FEU4C-25-L935 F4X-N-X-LI

COEFFICIENT OF UTILIZATION - ZONAL CAVITY METHOD:

RF	20				20				20				20				20
RC	80				70				50				30				0
RW	70	50	30	10	70	50	30	10	50	30	10		50	30	10		0
RCR																	
0	119	119	119	119	116	116	116	116	111	111	111		106	106	106		100
1	114	112	110	108	112	110	108	106	106	104	103		102	101	100		95
2	109	105	102	99	107	103	100	98	100	98	95		97	95	93		90
3	105	99	95	92	103	98	94	91	95	92	89		93	90	88		85
4	101	94	89	86	99	93	88	85	91	87	84		89	86	83		81
5	96	89	84	80	95	88	84	80	87	82	79		85	81	79		77
6	92	85	80	76	91	84	79	76	83	78	75		81	78	75		73
7	89	81	76	72	88	80	75	72	79	75	71		78	74	71		69
8	85	77	72	68	84	77	72	68	76	71	68		75	71	68		66
9	82	74	69	65	81	73	68	65	72	68	65		72	68	65		63
10	79	71	66	62	78	70	65	62	69	65	62		69	65	62		61

AVERAGE LUMINANCE (cd/sqm):

	0°
0°	693324
5°	623927
10°	483676
15°	350083
20°	242401
25°	176722
30°	128397
35°	75978
40°	31963
45°	9973
50°	1300
55°	728
60°	835
65°	988
70°	0
75°	0
80°	0
85°	0



TEST NUMBER: P696920
 CATALOG NUMBER: MRI-FEU4C-25-L935 F4X-N-X-LI

ZONAL LUMENS:

Zone	Lumens	% Fixture
0°-10°	444.7	20.3
10°-20°	761.4	34.7
20°-30°	605.1	27.6
30°-40°	320.3	14.6
40°-50°	55.2	2.5
50°-60°	4.2	0.2
60°-70°	2.1	0.1
70°-80°	0.0	0.0
80°-90°	0.0	0.0
90°-100°	0.0	0.0
100°-110°	0.0	0.0
110°-120°	0.0	0.0
120°-130°	0.0	0.0
130°-140°	0.0	0.0
140°-150°	0.0	0.0
150°-160°	0.0	0.0
160°-170°	0.0	0.0
170°-180°	0.0	0.0
0°-30°	1811.3	82.6
0°-40°	2131.6	97.2
0°-60°	2191.0	99.9
0°-90°	2193.0	100.0
90°-120°	0.0	0.0
90°-150°	0.0	0.0
90°-180°	0.0	0.0
0°-180°	2193.0	100.0

CANDELA DISTRIBUTION:

	0°	Flux
0°	5644	
5°	5059	445
15°	2752	761
25°	1304	605
35°	507	320
45°	57	55
55°	3	4
65°	3	2
75°	0	0
85°	0	0
90°	0	



TEST NUMBER: P696920
CATALOG NUMBER: MRI-FEU4C-25-L935 F4X-N-X-LI

CANDELA DISTRIBUTION (FULL):

0°	
0°	5643.5
2.5°	5498.2
5°	5059.3
7.5°	4485.1
10°	3877.2
12.5°	3289.6
15°	2752.5
17.5°	2252.6
20°	1854.1
22.5°	1550.1
25°	1303.7
27.5°	1104.4
30°	905.1
32.5°	702.5
35°	506.6
37.5°	334.4
40°	199.3
42.5°	114.9
45°	57.4
47.5°	20.3
50°	6.8
52.5°	6.8
55°	3.4
57.5°	3.4
60°	3.4
62.5°	3.4
65°	3.4
67.5°	0.0
70°	0.0
72.5°	0.0
75°	0.0
77.5°	0.0
80°	0.0
82.5°	0.0
85°	0.0
87.5°	0.0
90°	0.0

(END OF REPORT)